GIMA

PROFESSIONAL MEDICAL PRODUCTS

CINGHIE MONITOR FETALE SINGOLO PAZIENTE

SINGLE PATIENT FOETAL TRANSDUCER BELTS

SANGLES POUR TRANSDUCTEUR FOETAL À USAGE UNIQUE

CORREAS PACIENTE INDIVIDUAL PARA SONDA FETAL

CORREIA FETAL TRANSDUTORA DESCARTÁVEL

EINWEG-GÜRTEL FÜR FETALEN SCHALLKOPF

ΖΩΝΗ ΜΟΡΦΟΤΡΟΠΕΑ ΕΜΒΡΥΪΚΟΥ ΕΛΕΓΧΟΥ ΜΙΑΣ ΧΡΗΣΗΣ

EENMALIGE FOETALE TRANSDUCER RIEM

PASEK PRZETWORNIKA PŁODU JEDNORAZOWEGO UŻYTKU

CUREA ABDOMINALĂ PENTRU MONITORIZARE FETALĂ, DE UNICĂ FOLOSINȚĂ


FOSTERGIVAREBÄLTE FÖR ENGÅNGSBRUK

GIMA 29544

REF B01

Fabbricante / Manufacturer / Fabricant / Fabricante / Fabricante / Hersteller / Κατασκευαστής / Fabrikant / Producent / Producător / Tillverkare:
Dongguan Belcare Medical Technology Co., Ltd.
503 of 2nd. Block, #2 of Shaping Road,Tangxia Town,
Dongguan, Guangdong, China 523710 - joe@belcare-med.com
Made in China

Importato da/Imported by/ Importé par/ Importiert von/ Importado por/ Importado por/ Εισάγεται ααπό / Geïmporteerd door / Importowane przez / Importat de / Importerad av:
Gima S.p.A.
Via Marconi, 1 - 20060 Gessate (MI) Italy
gima@gimaitaly.com - export@gimaitaly.com
www.gimaitaly.com

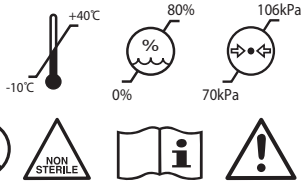

M29544-M-rev.1-11.24

Intended use:

• This product works according to adjust buckle's place on the belt to fix the fetal transducer.

Product introduction:

• Product name: Disposable fetal transducer belt.

• Product structure: It's made up of elastic belt and buckle.

Product range:

• It used with fetal transducer when pregnant in fetal monitoring, to fix the fetal transducer.

Use condition:

• Temperature: 0°C~40°C

• Relative humidity: 15%~95%

• Atmospheric pressure: 70kpa~106kpa

Package and storage:

• Disposable fetal belt should be single packaged, packaged product should be stored in a non-corrosive gas, good ventilation room.

Store environment as below:

• Temperature: -10°C~+40°C

• Relative humidity: ≤80%

• Atmospheric pressure:70kpa~106kpa

Installation/use:

• Attach one end of the belt to the transducer by engaging one of the holes in the belt over the button on the top of the transducer.

• Keeping the transducer in position, tension the other end of the belt and engage the belt over the button, ensuring sufficient tension to keep the transducer in firm contact with the abdomen.

• Avoid over-tightening as this will cause unnecessary discomfort to the patient.

Product clean:

• Wash belt in warm water, do not rub the edge fetal belt to avoid removal, do not exposure.

Validity period:

• Validity period: 2 years.

Replace and abandon:

• Replace: Under these situations such as fracture, elastic damage, expiry date, please change new fetal belt to use.

• Abandon: Abandoned belt can be processed as normal waste.

Contraindications, precautions, warnings and cautionary statements:

• Contraindications: The belts must not be fixed at the injury site.

• Spandex allergies to stop using.

• Cautionary statements: This product is a single-use products to avoid cross infection. Please read the instructions before use.

GIMA WARRANTY TERMS

The Gima 12-month standard B2B warranty applies

