PENCIL

REF 00201.02_S

Handle for microsurgical needle autoclavable

LOT 000000 YYYY-MM YYYY-MM

for MICRO-NEEDLE Ø 1mm 00500.L11
(500500.L11 blister pack 10 pcs)

NON STERILE

134°C

CICLI 100 CYCLES

04 PE-LD

INTENDED USE:

Medical devices reserved for use by specialized medical personnel intended for temporary use for surgical operations in which, through connection to electrosurgical units, cutting and / or coagulation of soft tissues is required, with a monopolar and / or bipolar technique, for minor surgery and / or major in open and / or intra-operative percutaneous and / or endoscopic and / or laparoscopic.

Warning:

•The following precautions reduce the risk of accidental burnings.
• The product must be used with ESU and/or accessories comply with current regulations.
• The micro-needle electrode must be reliably connected to the handpiece, to secure / disconnect see figure.
• Do not let the wires come into direct contact with the patient's skin, a capacitive effect could cause burns.
• When removing, do not pull the cable straight away but act on the provided connector.
• Always check the return plate whenever unit fails to produce the desired effect. Reason for a low output power level, or for an incorrect functioning of the unit when arranged for a normal output, may be lack of connection of the return plate or its imperfect placement.
•The user and/or the patient shall be informed of the need to report any serious incident that has occurred in relation to the device, the manufacturer and the competent authority of the Member State where the user is established.

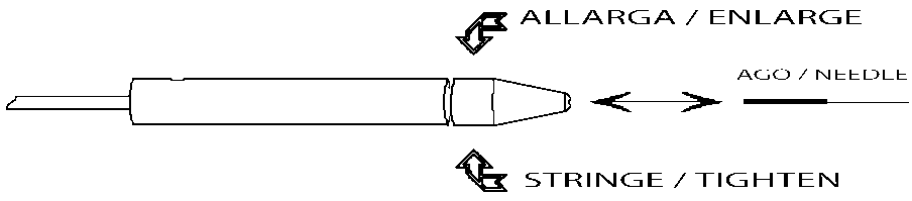

UDI 8 033638 323809

SURGEON

LED SpA Via M.T. Cicerone 138

03100 Frosinone (FR) - ITALY

CE 0051 MD

MADE IN ITALY

IA00201.02_S_a_EN ed. 2023-02